

# Hydrophobicity of artificial eye surfaces before and after cleaning.

Keith Pine BSc, MBA, MIMPT  
PhD candidate, The University of Auckland  
Supervisors: Dr R. Jacobs & Dr B. Sloan.

## Background

Cleaning regimes are associated with discharge frequency and volume but the direction of the effect has not been found.

## Aim

The aim of this experiment was to measure the hydrophobicity of artificial eye surfaces before and after cleaning and removal of surface deposits.

## Method

18 anophthalmic patients were recruited. The wetting angles on the surface of their artificial eyes were measured by a goniometer using plain water droplets. The measurements were taken before and after wiping the surface with paper towel wetted with cold water. Statistical analysis was carried out using a 2 sample t-test assuming unequal variances.

## Results

The mean of the wetting angles before cleaning was  $29.8^\circ$  and after cleaning it was  $80.8^\circ$  ( $p < 0.0001$ ).


## Conclusions

The finding that hydrophobicity levels rose significantly after artificial eyes were cleaned suggests that the tear film is likely to break up when the eye is re-inserted in the socket. The resulting dry areas may mildly irritate the conjunctiva leading to the production of mucins and increased discharge.

The result of this experiment provides causal evidence for the finding that more frequent cleaning is associated with more severe discharge. This is an important outcome because discharge is the main current concern for anophthalmic patients after health of the remaining eye\*.




A water droplet is being syringed on to an artificial eye set up in a goniometer.



The wetting angle,  $\theta_C$ , is the angle formed by the water droplet at the three phase boundary where the water, air, and artificial eye surface intersect.

Wetting angles on artificial eyes before and after cleaning.

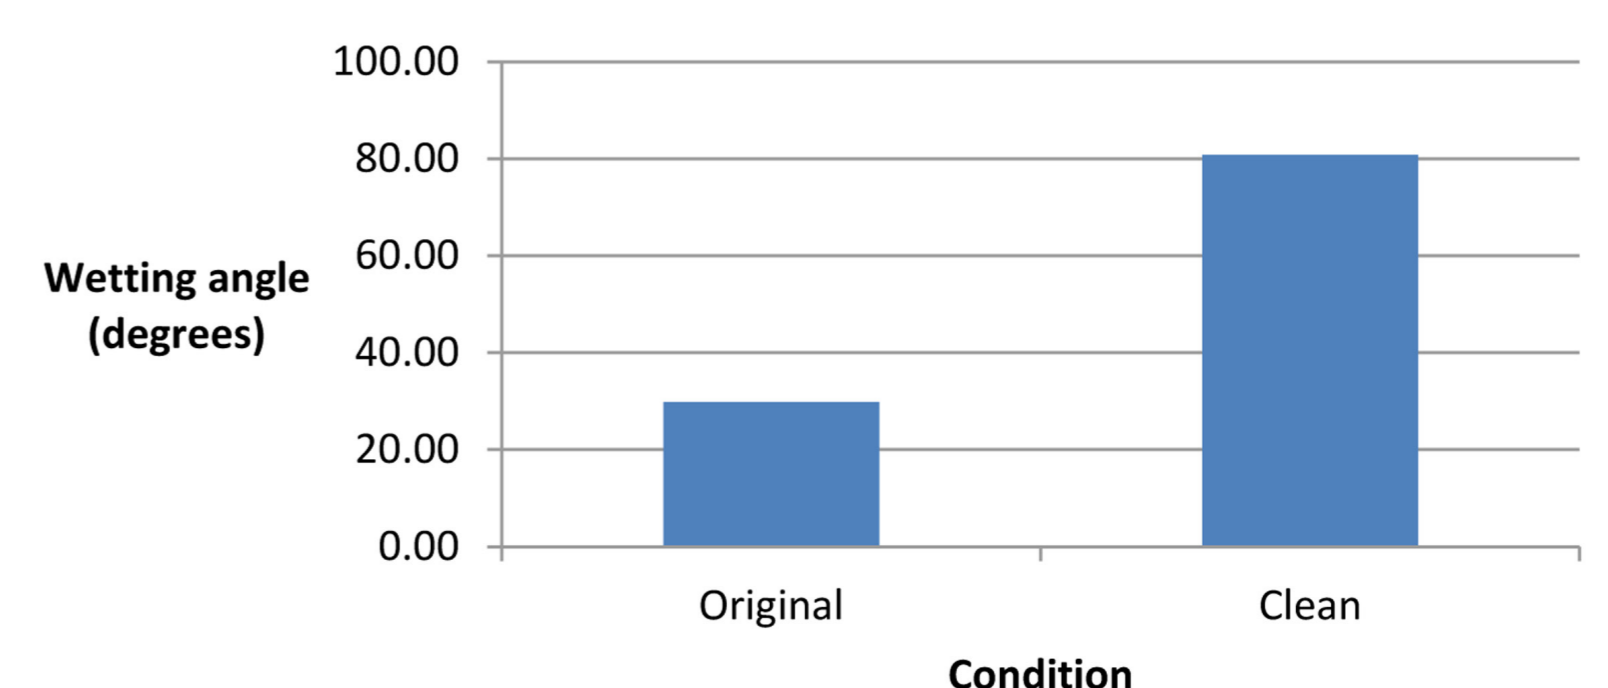

Surface hydrophobicity increased significantly after cleaning.